Safe-Flo™

Saliva Ejectors and Valves

Protect your patients from evacuation line backflow

Evacuation line health risk is real

Backflow in low-volume evacuation lines can occur when the pressure in the patient's mouth is less than in the evacuator. This condition can result under several commonly occurring situations[1]:


- Patient creates a seal around the saliva ejector by closing their lips around the tip
- Saliva ejector tip becomes occluded from cheek, tongue or other blockage
- Suction tubing is positioned above the patient's mouth
- Simultaneous use of other evacuation (HV) equipment

Patient Safety

Keep all your patients safe from the potential risk of contaminated backflow. Provides added protection for geriatric patients who may experience a variety of oral soft tissue changes, as well as pediatric and special needs patients who may inadvertently close their lips around the saliva ejector.

Patented Backflow Prevention[2]

The unique, one-way valve provides a physical barrier to prevent backflow from occurring.

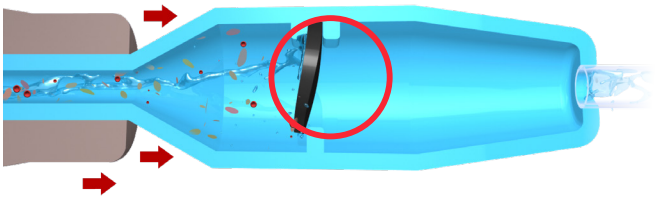


Seamless Workflow

The integrity of suction and performance of the saliva ejector or HVE tip is not affected, so there is no need to change how you work in order to protect from backflow.

NEW Safe-Flo™ Plus Saliva Ejectors

- Featuring our popular Comfort Plus™ Saliva Ejector tip—rounded, smooth design with strategically placed ports for optimal suction.
- For backflow prevention in low-volume evacuation lines.
- Fully assembled, all-in-one saliva ejector with Safe-Flo™ Valve replaces your current saliva ejector brand.

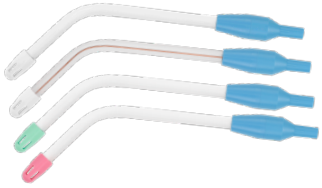




Safe-Flo™ Saliva Ejectors

- For backflow prevention in low-volume evacuation lines.
- Fully assembled, all-in-one saliva ejector with Safe-Flo™ Valve replaces your current saliva ejector brand.




Safe-Flo™ Saliva Ejector Valve

- For backflow prevention in low-volume evacuation lines.
- Use with your preferred saliva ejector brand.




Safe-Flo™ High Volume Evacuation Valve

- For backflow prevention in high-volume evacuation (HVE) lines.
- Use with your preferred HVE tip brand.



Safe-Flo™ Adapter

- Allows you to use the HVE line with your preferred saliva ejector brand for backflow prevention.
- Provides a higher level of aspiration to the saliva ejector.




HuFriedyGroup
The Best In Practice

Safe-Flo™
Saliva Ejectors and Valves


DID YOU KNOW?

Studies show contaminated **backflow could potentially occur 21% of the time**[3]. Safe-Flo™ Saliva Ejectors and Valves provide backflow prevention you can rely on to protect all of your patients.

Backflow may contain:



Safe-Flo™ Saliva Ejectors and Valves are available as a complete saliva ejector/valve system or sold separately for use with your preferred brand of saliva ejectors or HVE tips.

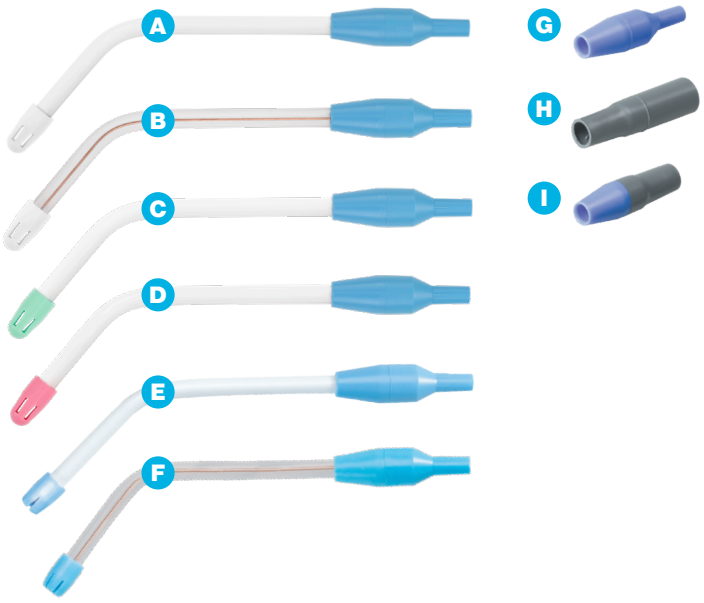

	Description	Quantity	Part Code
A	**NEW Safe-Flo™ Plus Saliva Ejector, White/White**	100/Bag	**M1002WHWH**
B	**NEW Safe-Flo™ Plus Saliva Ejector, Clear/White**	100/Bag	**M1003CLWH**
C	**NEW Safe-Flo™ Plus Saliva Ejector, White/Green, Mint Scented**	100/Bag	**M1004WHGR**
D	**NEW Safe-Flo™ Plus Saliva Ejector, White/Pink, Bubblegum Scented**	100/Bag	**M1005WHPK**
E	**Safe-Flo™ Saliva Ejector, White/Blue**	100/Bag	**M1000WHBU**
F	**Safe-Flo™ Saliva Ejector, Clear/Blue**	100/Bag	**M1001CLBU**
G	**Safe-Flo™ SE Valve, Blue**	100/Bag	**M1010SUSE**
H	**Safe-Flo™ HV Valve, Gray**	100/Bag	**M1030HVSE**
I	**Safe-Flo™ Adapter, Blue/Gray**	50/Bag	**M1020ADAP**

Use a Safe-Flo™ Valve with any evacuation line.

Low Volume



High Volume



Safe-Flo™ Valves are single-use disposable, one-way valves that stop backflow from evacuation lines, preventing cross-contamination.

Call your preferred distributor to order, or learn more at **HuFriedyGroup.com/Safe-Flo**

MADE IN USA

Not made with natural rubber latex.

1) Center for Disease Control and Prevention. Guidelines for Infection Control in Dental Health Care Settings-2003. MMWR 2003:52 (no. RR-17); [31].
2) US Pat. No. 8,256,464, 8,714,200, 8,752,579 and foreign counterparts.
3) Miller C. Back flow in low-volume suction lines may lead to potential cross-contamination. RDH. 1996; 16(1):30.

All company and product names are trademarks of Hu-Friedy Mfg. Co., LLC, its affiliates or related companies, unless otherwise noted. Marks not registered in all jurisdictions. HuFriedyGroup.com
©2026 Hu-Friedy Mfg. Co., LLC. All rights reserved. HFL-807 / 2607

HuFriedyGroup
The Best In Practice